

Certificate number: o60224369i246275-A-1



# Calibration Certificate



Customer  
UPSTATE MEDICAL PHYSICS  
BLOSSOM DR 1290  
13078 JAMESVILLE  
US

Laboratory  
Unfors RaySafe Inc.  
2 Science Road  
Glenwood, IL 60425-1586  
USA  
+1-833-296-9240  
customerservice.us@raysafe.com

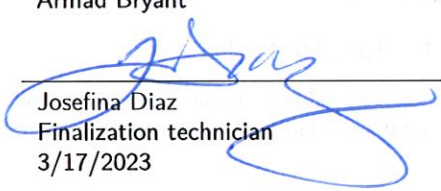
## CUSTOMER INSTRUMENT

Product X2 R/F  
Serial number 246275  
Manufacturer RaySafe

## CALIBRATION INFORMATION

As found 3/7/2023  
As left 3/10/2023  
Adjustment done Yes  
Tested by Amber Ramos  
Armada Bryant

Approved by

  
Josefina Diaz  
Finalization technician

Certificate date 3/17/2023

## CALIBRATION RESULT

AS FOUND: All measured and tested values of this certificate were found to be in conformance with the specification.

AS LEFT: All measured and tested values of this certificate were found to be in conformance with the specification.

Relevant instrument specifications

Air kerma: 5 %, Air kerma rate: 5 %  
Time: 0.5 %, Voltage: 2 %

This laboratory is accredited according to ISO/IEC 17025:2017 by the American Association for Laboratory Accreditation (A2LA) and the results shown in this certificate have been determined within the scope of accreditation unless stated otherwise in this certificate.



Certificate number: o60224369i246275-B-1



# Calibration Certificate

Customer  
UPSTATE MEDICAL PHYSICS  
BLOSSOM DR 1290  
13078 JAMESVILLE  
US

Laboratory  
Unfors RaySafe Inc.  
2 Science Road  
Glenwood, IL 60425-1586  
USA  
+1-833-296-9240  
customerservice.us@raysafe.com

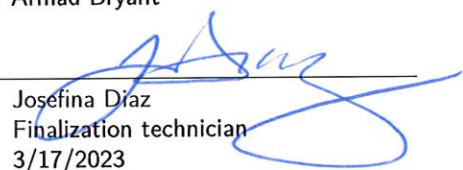
## CUSTOMER INSTRUMENT

Product X2 R/F  
Serial number 246275  
Manufacturer RaySafe

## CALIBRATION INFORMATION

As found 3/7/2023  
As left 3/10/2023  
Adjustment done Yes  
Tested by Amber Ramos  
Armad Bryant

Approved by

  
Josefina Díaz  
Finalization technician

Certificate date 3/17/2023



Certificate number: o60224765i279246-A-1



# Calibration Certificate



Customer  
UPSTATE MEDICAL PHYSICS  
BLOSSOM DR 1290  
13078 JAMESVILLE  
US

Laboratory  
Unfors RaySafe Inc.  
2 Science Road  
Glenwood, IL 60425-1586  
USA  
+1-833-296-9240  
customerservice.us@raysafe.com

## CUSTOMER INSTRUMENT

Product X2 MAM  
Serial number 279246  
Manufacturer RaySafe

## CALIBRATION INFORMATION

As found 3/14/2023  
As left 3/16/2023  
Adjustment done Yes  
Tested by Channell Kennedy  
Elijah Thompson  
Tommy Cox

Approved by

Josefina Diaz  
Finalization technician

Certificate date

3/17/2023

## CALIBRATION RESULT

AS FOUND: All measured and tested values of this certificate were found to be in conformance with the specification.

AS LEFT: All measured and tested values of this certificate were found to be in conformance with the specification.

Relevant instrument specifications

Air Kerma: 5 %

Voltage: 2 % or 0.5 kV (without paddle), 2 % or 0.7 kV (with paddle)

This laboratory is accredited according to ISO/IEC 17025:2017 by the American Association for Laboratory Accreditation (A2LA) and the results shown in this certificate have been determined within the scope of accreditation unless stated otherwise in this certificate.



Certificate number: o60224765i279246-B-1



# Calibration Certificate

Customer  
UPSTATE MEDICAL PHYSICS  
BLOSSOM DR 1290  
13078 JAMESVILLE  
US

Laboratory  
Unfors RaySafe Inc.  
2 Science Road  
Glenwood, IL 60425-1586  
USA  
+1-833-296-9240  
customerservice.us@raysafe.com


## CUSTOMER INSTRUMENT

Product X2 MAM  
Serial number 279246  
Manufacturer RaySafe

## CALIBRATION INFORMATION

As found 3/14/2023  
As left 3/16/2023  
Adjustment done Yes  
Tested by Channell Kennedy  
Elijah Thompson  
Tommy Cox

Approved by

  
Josefina Diaz  
Finalization technician

Certificate date

3/17/2023





Certificate number: o60224513i229933-1



# Calibration Certificate



Customer  
UPSTATE MEDICAL PHYSICS  
BLOSSOM DR 1290  
13078 JAMESVILLE  
US

Laboratory  
Unfors RaySafe Inc.  
2 Science Road  
Glenwood, IL 60425-1586  
USA  
+1-833-296-9240  
customerservice.us@raysafe.com

## CUSTOMER INSTRUMENT

Product X2 Survey  
Serial number 229933  
Manufacturer RaySafe

## CALIBRATION INFORMATION

As found 3/8/2023  
As left 3/13/2023  
Adjustment done Yes  
Tested by Amber Ramos  
Joseph Hertl

Approved by

Josefina Diaz  
Finalization technician

Certificate date

3/17/2023

## CALIBRATION RESULT

AS FOUND: All measured and tested values of this certificate were found to be in conformance with the specification.

AS LEFT: All measured and tested values of this certificate were found to be in conformance with the specification.

Relevant instrument specifications

Air kerma: 5 % (RQA), 10 % (N-series)

This laboratory is accredited according to ISO/IEC 17025:2017 by the American Association for Laboratory Accreditation (A2LA) and the results shown in this certificate have been determined within the scope of accreditation unless stated otherwise in this certificate.



Certificate number: o60224568i224328-1



# Calibration Certificate



Customer  
UPSTATE MEDICAL PHYSICS  
BLOSSOM DR 1290  
13078 JAMESVILLE  
US

Laboratory  
Unfors RaySafe Inc.  
2 Science Road  
Glenwood, IL 60425-1586  
USA  
+1-833-296-9240  
customerservice.us@raysafe.com

## CUSTOMER INSTRUMENT

Product X2 CT  
Serial number 224328  
Manufacturer RaySafe

## CALIBRATION INFORMATION

As found 3/9/2023  
As left 3/9/2023  
Adjustment done Yes  
Tested by Amber Ramos

Approved by

\_\_\_\_\_  
Josefina Diaz  
Finalization technician  
3/17/2023

## CALIBRATION RESULT

AS FOUND: All measured and tested values of this certificate were found to be in conformance with the specification.  
AS LEFT: All measured and tested values of this certificate were found to be in conformance with the specification.

Relevant instrument specifications

Air kerma: 5 %

This laboratory is accredited according to ISO/IEC 17025:2017 by the American Association for Laboratory Accreditation (A2LA) and the results shown in this certificate have been determined within the scope of accreditation unless stated otherwise in this certificate.



Certificate number: o60224535i288586-1



# Calibration Certificate

Customer  
UPSTATE MEDICAL PHYSICS  
BLOSSOM DR 1290  
13078 JAMESVILLE  
US

Laboratory  
Unfors RaySafe Inc.  
2 Science Road  
Glenwood, IL 60425-1586  
USA  
+1-833-296-9240  
customerservice.us@raysafe.com


## CUSTOMER INSTRUMENT

Product X2 Light  
Serial number 288586  
Manufacturer RaySafe

## CALIBRATION INFORMATION

As found 3/9/2023  
As left 3/10/2023  
Adjustment done Yes  
Tested by Joseph Hertl

Approved by

  
Josefina Diaz  
Finalization technician

Certificate date 3/17/2023

## CALIBRATION RESULT

**AS FOUND:** One or more measured and tested values of this certificate are within the specifications by a margin less than the expanded measurement uncertainty. Therefore, it is not possible to state conformance with specifications for those measurements.

**AS LEFT:** All measured and tested values of this certificate were found to be in conformance with the specification.

Relevant instrument specifications

Illuminance: 3 %  
Luminance: 3 %

