

Certificate number: o60234773i322143-A-1



Calibration Certificate



Customer
UPSTATE MEDICAL PHYSICS
BLOSSOM DR 1290
14564 VICTOR
US

Laboratory
Unfors RaySafe Inc.
2 Science Road
Glenwood, IL 60425-1586
USA
+1-833-296-9240
customerservice.us@raysafe.com

CUSTOMER INSTRUMENT

Product X2 R/F
Serial number 322143
Manufacturer RaySafe

CALIBRATION INFORMATION

As found Not performed
As left 12/21/2023
Adjustment done Yes
Tested by Armad Bryant

Approved by

Josefina Diaz
Finalization technician

Certificate date

12/29/2023

CALIBRATION RESULT

AS LEFT: All measured and tested values of this certificate were found to be in conformance with the specification.

Relevant instrument specifications

Air kerma: 5 %, Air kerma rate: 5 %
Time: 0.5 %, Voltage: 2 %

This laboratory is accredited according to ISO/IEC 17025:2017 by the American Association for Laboratory Accreditation (A2LA) and the results shown in this certificate have been determined within the scope of accreditation unless stated otherwise in this certificate.



Certificate number: o60234773i322143-B-1



Calibration Certificate

Customer
UPSTATE MEDICAL PHYSICS
BLOSSOM DR 1290
14564 VICTOR
US

Laboratory
Unfors RaySafe Inc.
2 Science Road
Glenwood, IL 60425-1586
USA
+1-833-296-9240
customerservice.us@raysafe.com

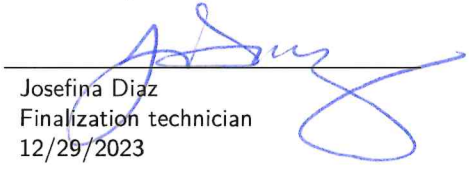
CUSTOMER INSTRUMENT

Product X2 R/F
Serial number 322143
Manufacturer RaySafe

CALIBRATION INFORMATION

As found	Not performed
As left	12/21/2023
Adjustment done	Yes
Tested by	Armad Bryant

Approved by


Josefina Diaz
Finalization technician

Certificate date

12/29/2023



Calibration Certificate



Customer
UPSTATE MEDICAL PHYSICS
BLOSSOM DR 1290
14564 VICTOR
US

Laboratory
Unfors RaySafe Inc.
2 Science Road
Glenwood, IL 60425-1586
USA
+1-833-296-9240
customerservice.us@raysafe.com

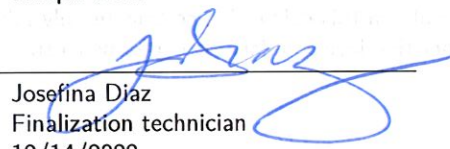
CUSTOMER INSTRUMENT

Product X2 Survey
Serial number 230023
Manufacturer RaySafe

CALIBRATION INFORMATION

As found 12/7/2022
As left 12/8/2022
Adjustment done Yes
Tested by Channell Kennedy
Joseph Hertl

Approved by


Josefina Diaz
Finalization technician

Certificate date 12/14/2022

CALIBRATION RESULT

AS FOUND: All measured and tested values of this certificate were found to be in conformance with the specification.

AS LEFT: All measured and tested values of this certificate were found to be in conformance with the specification.

Relevant instrument specifications

Air kerma: 5 % (RQA), 10 % (N-series)

This laboratory is accredited according to ISO/IEC 17025:2017 by the American Association for Laboratory Accreditation (A2LA) and the results shown in this certificate have been determined within the scope of accreditation unless stated otherwise in this certificate.



Certificate number: o60221231i272789-1



Calibration Certificate

Customer
UPSTATE MEDICAL PHYSICS
BLOSSOM DR 1290
14564 VICTOR
US

Laboratory
Unfors RaySafe Inc.
2 Science Road
Glenwood, IL 60425-1586
USA
+1-833-296-9240
customerservice.us@raysafe.com

CUSTOMER INSTRUMENT

Product X2 Light
Serial number 272789
Manufacturer RaySafe

CALIBRATION INFORMATION

As found 12/7/2022
As left 12/13/2022
Adjustment done Yes
Tested by Elijah Thompson
Nate Barnes

Approved by

Josefina Diaz
Finalization technician
12/14/2022

CALIBRATION RESULT

AS FOUND: One or more measured and tested values of this certificate are outside of the specifications by a margin less than the expanded measurement uncertainty. Therefore, it is not possible to state non-conformance with specifications for those measurements.

AS LEFT: All measured and tested values of this certificate were found to be in conformance with the specification.

Relevant instrument specifications

Illuminance: 3 %
Luminance: 3 %



Certificate number: o60221279i246298-B-1



Calibration Certificate

Customer
UPSTATE MEDICAL PHYSICS
BLOSSOM DR 1290
14564 VICTOR
US

Laboratory
Unfors RaySafe Inc.
2 Science Road
Glenwood, IL 60425-1586
USA
+1-833-296-9240
customerservice.us@raysafe.com

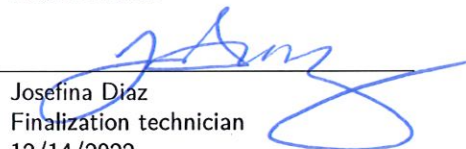
CUSTOMER INSTRUMENT

Product X2 R/F
Serial number 246298
Manufacturer RaySafe

CALIBRATION INFORMATION

As found 12/7/2022
As left 12/10/2022
Adjustment done Yes
Tested by Amber Ramos
Kierra Sullivan

Approved by


Josefina Diaz
Finalization technician

Certificate date

12/14/2022



Certificate number: o60221279i246298-A-1



Calibration Certificate



Customer
UPSTATE MEDICAL PHYSICS
BLOSSOM DR 1290
14564 VICTOR
US

Laboratory
Unfors RaySafe Inc.
2 Science Road
Glenwood, IL 60425-1586
USA
+1-833-296-9240
customerservice.us@raysafe.com

CUSTOMER INSTRUMENT

Product X2 R/F
Serial number 246298
Manufacturer RaySafe

CALIBRATION INFORMATION

As found 12/7/2022
As left 12/10/2022
Adjustment done Yes
Tested by Amber Ramos
Kierra Sullivan

Approved by

Josefina Diaz
Finalization technician

Certificate date

12/14/2022

CALIBRATION RESULT

AS FOUND: All measured and tested values of this certificate were found to be in conformance with the specification.

AS LEFT: All measured and tested values of this certificate were found to be in conformance with the specification.

Relevant instrument specifications

Air kerma: 5 %, Air kerma rate: 5 %

Time: 0.5 %, Voltage: 2 %

This laboratory is accredited according to ISO/IEC 17025:2017 by the American Association for Laboratory Accreditation (A2LA) and the results shown in this certificate have been determined within the scope of accreditation unless stated otherwise in this certificate.

