


Certificate number: o60238927i279575-A-1



Calibration Certificate



Customer
UPSTATE MEDICAL PHYSICS
BLOSSOM 1290
14564 VICTOR
US

Laboratory
Unfors RaySafe Inc.
2 Science Road
Glenwood, IL 60425-1586
USA
+1-833-296-9240
customerservice.us@raysafe.com


CUSTOMER INSTRUMENT

Product X2 R/F
Serial number 279575
Manufacturer RaySafe

CALIBRATION INFORMATION

As found 4/15/2024
As left 4/18/2024
Adjustment done Yes
Tested by Rosio Ramos

Approved by

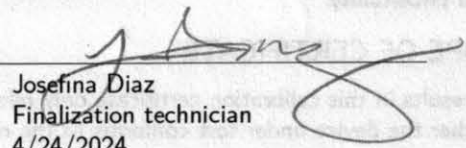
Josefina Diaz
Finalization technician

Certificate date 4/24/2024

CALIBRATION RESULT

AS FOUND: All measured and tested values of this certificate were found to be in conformance with the specification.

AS LEFT: All measured and tested values of this certificate were found to be in conformance with the specification.


Relevant instrument specifications

Air kerma: 5 %, Air kerma rate: 5 %
Time: 0.5 %, Voltage: 2 %

This laboratory is accredited according to ISO/IEC 17025:2017 by the American Association for Laboratory Accreditation (A2LA) and the results shown in this certificate have been determined within the scope of accreditation unless stated otherwise in this certificate.



Certificate number: o60238927i279575-B-1



Calibration Certificate

GENERAL INFORMATION

LABORATORY CALIBRATION

All reference standards used for this calibration are valid for one year. All other time intervals are subject to change. All Air kerma and dose rate standards are traceable to Physikalisch-Technische Bundesanstalt (PTB). All standards are traceable to PTB and PTB.

CALIBRATION ENVIRONMENTAL CONDITIONS

Customer
UPSTATE MEDICAL PHYSICS
BLOSSOM 1290
14564 VICTOR
US

Laboratory
Unfors RaySafe Inc.
2 Science Road
Glenwood, IL 60425-1586
USA
+1-833-296-9240
customerservice.us@raysafe.com


CUSTOMER INSTRUMENT

Product X2 R/F
Serial number 279575
Manufacturer RaySafe

CALIBRATION INFORMATION

As found 4/15/2024
As left 4/18/2024
Adjustment done Yes
Tested by Rosio Ramos

Approved by

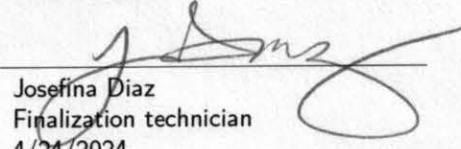
Josefina Diaz
Finalization technician

Certificate date 4/24/2024



Calibration Certificate



Customer
UPSTATE MEDICAL PHYSICS
BLOSSOM 1290
14564 VICTOR
US

Laboratory
Unfors RaySafe Inc.
2 Science Road
Glenwood, IL 60425-1586
USA
+1-833-296-9240
customerservice.us@raysafe.com

CUSTOMER INSTRUMENT

Product X2 MAM
Serial number 279216
Manufacturer RaySafe

CALIBRATION INFORMATION

As found 4/9/2024
As left 4/17/2024
Adjustment done Yes
Tested by America Arroyo
Christina Arroyo
Rosio Ramos

Approved by

Josefina Diaz
Finalization technician

Certificate date

4/24/2024

CALIBRATION RESULT

AS FOUND: One or more measured and tested values of this certificate are within the specifications by a margin less than the expanded measurement uncertainty. Therefore, it is not possible to state conformance with specifications for those measurements.

AS LEFT: All measured and tested values of this certificate were found to be in conformance with the specification.

Relevant instrument specifications


Air Kerma: 5 %

Voltage: 2 % or 0.5 kV (without paddle), 2 % or 0.7 kV (with paddle)

This laboratory is accredited according to ISO/IEC 17025:2017 by the American Association for Laboratory Accreditation (A2LA) and the results shown in this certificate have been determined within the scope of accreditation unless stated otherwise in this certificate.



Certificate number: o60238695i279216-B-1



Calibration Certificate

GENERAL INFORMATION

LABORATORY CALIBRATION

All services standards used for the calibration are valid for one year. Validity may be extended only if the instrument is used for the same purpose. All services standards are traceable to NIST Special Publication 400-11. All services standards are traceable to NIST Special Publication 400-11. All services standards are traceable to NIST Special Publication 400-11.

CALIBRATION ENVIRONMENTAL CONDITIONS

Customer
UPSTATE MEDICAL PHYSICS
BLOSSOM 1290
14564 VICTOR
US

Laboratory
Unfors RaySafe Inc.
2 Science Road
Glenwood, IL 60425-1586
USA
+1-833-296-9240
customerservice.us@raysafe.com


CUSTOMER INSTRUMENT

Product X2 MAM
Serial number 279216
Manufacturer RaySafe

CALIBRATION INFORMATION

As found 4/9/2024
As left 4/17/2024
Adjustment done Yes
Tested by America Arroyo
Christina Arroyo
Rosio Ramos

Approved by

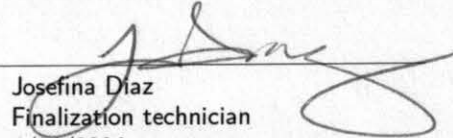

Josefina Diaz
Finalization technician

Certificate date

4/24/2024



Certificate number: o60238836i263036-1



Calibration Certificate



Customer
UPSTATE MEDICAL PHYSICS
BLOSSOM 1290
14564 VICTOR
US

Laboratory
Unfors RaySafe Inc.
2 Science Road
Glenwood, IL 60425-1586
USA
+1-833-296-9240
customerservice.us@raysafe.com


CUSTOMER INSTRUMENT

Product X2 Survey
Serial number 263036
Manufacturer RaySafe

CALIBRATION INFORMATION

As found 4/12/2024
As left 4/12/2024
Adjustment done Yes
Tested by Amber Ramos

Approved by

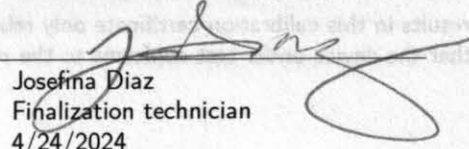
Josefina Diaz
Finalization technician

Certificate date 4/24/2024

CALIBRATION RESULT

AS FOUND: All measured and tested values of this certificate were found to be in conformance with the specification.

AS LEFT: All measured and tested values of this certificate were found to be in conformance with the specification.


Relevant instrument specifications

Air kerma: 5 % (RQA), 10 % (N-series)

This laboratory is accredited according to ISO/IEC 17025:2017 by the American Association for Laboratory Accreditation (A2LA) and the results shown in this certificate have been determined within the scope of accreditation unless stated otherwise in this certificate.



Certificate number: o60238734i293251-1



Calibration Certificate



Customer
UPSTATE MEDICAL PHYSICS
BLOSSOM 1290
14564 VICTOR
US

Laboratory
Unfors RaySafe Inc.
2 Science Road
Glenwood, IL 60425-1586
USA
+1-833-296-9240
customerservice.us@raysafe.com


CUSTOMER INSTRUMENT

Product X2 CT
Serial number 293251
Manufacturer RaySafe

CALIBRATION INFORMATION

As found 4/10/2024
As left 4/10/2024
Adjustment done Yes
Tested by Amber Ramos

Approved by

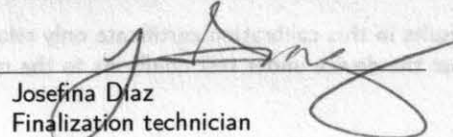
Josefina Diaz
Finalization technician

Certificate date 4/24/2024

CALIBRATION RESULT

AS FOUND: All measured and tested values of this certificate were found to be in conformance with the specification.

AS LEFT: All measured and tested values of this certificate were found to be in conformance with the specification.

Relevant instrument specifications

Air kerma: 5 %

This laboratory is accredited according to ISO/IEC 17025:2017 by the American Association for Laboratory Accreditation (A2LA) and the results shown in this certificate have been determined within the scope of accreditation unless stated otherwise in this certificate.



Certificate number: o60238691i272670-1

Calibration Certificate

Customer
UPSTATE MEDICAL PHYSICS
BLOSSOM 1290
14564 VICTOR
US

Laboratory
Unfors RaySafe Inc.
2 Science Road
Glenwood, IL 60425-1586
USA
+1-833-296-9240
customerservice.us@raysafe.com


CUSTOMER INSTRUMENT

Product X2 Light
Serial number 272670
Manufacturer RaySafe

CALIBRATION INFORMATION

As found 4/9/2024
As left 4/10/2024
Adjustment done Yes
Tested by Nate Barnes

Approved by

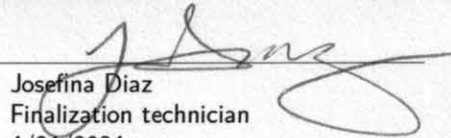

Josefina Diaz
Finalization technician

Certificate date 4/24/2024

CALIBRATION RESULT

AS FOUND: One or more measured and tested values of this certificate are within the specifications by a margin less than the expanded measurement uncertainty. Therefore, it is not possible to state conformance with specifications for those measurements.

AS LEFT: All measured and tested values of this certificate were found to be in conformance with the specification.

Relevant instrument specifications

Illuminance: 3 %
Luminance: 3 %

